

The Influence of Heat Treatment on the Mechanical Properties of 3D-Printed Cobalt-Chrome Alloy Used in Dental Laboratory Practice

Klaudia KULCSÁR,¹ János KÓNYA²

Dent-Art-Technik Kft., Győr, Hungary

¹ kulcsar.klaudia@dentarttechnik.hu

² janos@dentarttechnik.hu

Abstract

The material used for manufacturing of dental implantation prostheses is cobalt-chromium alloy. The following study presents a new heat treatment technology for dental implantation prostheses. Specimens were created with the innovative technology of 3D printing. The brittleness of specimens subjected to heat treatment with parameters recommended by the manufacturer made it necessary for us to reconsider the heat-treating process. After changing given heat treatment processes, tensile and hardness tests were performed. From these tests, the optimal heat treatment process technology was chosen.

Keywords: *cobalt-chrome alloy, heat treatment, 3D printing.*

1. Introduction

In recent decades, cobalt-chromium alloys have been widely used in casting molds due to their outstanding corrosion resistance, bio-compatibility, and strength [1–3]. Over the years, cobalt-chromium (Co-Cr) alloys have shown remarkable versatility and durability as orthopaedic implant materials [4]. Co-Cr alloys are also used in dental practice e.g. abutments (superstructures), crowns, and bridges [5]. These alloys provide the best balance between mechanical strength and wear resistance. Moreover, their corrosion resistance is also remarkable [6–10]. In the dental field, conventional lost-wax casting techniques have been used for decades. However, these techniques are susceptible to human errors [11]. The production of dental implants is common with conventional methods, for example casting technology [12]. Precision casting and forging still belong to conventional methods in terms of implant manufacturing [13]. On the other hand, additive manufacturing technologies are becoming even more widespread in the production of dental implant prostheses [14]. To make SLM technology suitable for implant or prosthesis manufacturing, certain condi-

tions must be met. The mechanical and chemical properties of the layers created with laser melting of particles must match strict requirements [15]. Mechanical properties and corrosion resistance of alloys processed with SLM (Selective Laser Melting) were studied [16]. Moreover, the strength of the adhesion bond between the ceramic material and Co-Cr alloy was also examined [17].

2. Materials and methods

2.1. Materials used

Type 5, ISO 22674, and ISO 9693-1 dental Co-Cr alloy were used. The chemical composition (% by weight) of cobalt-chromium is shown in Table 1.

Table 1. Chemical composition of Co-Cr alloy

Element	% by weight
Cobalt (Co)	63.9
Chromium (Cr)	24.7
Tungsten (W)	5.4
Molybdenum (Mo)	5.0
Silicon (Si)	1.0

2.2. 3D printing of specimens

Co63.9Cr24.7W5.4Mo5.0Si1.0 (%) alloy can be the material of choice for implants and prostheses created with additive manufacturing processes. Test specimens were manufactured with a Sisma Mysint 3D printer. 3D printing is carried out with LMF (Laser Metal Fusion) technology. This technology requires a specific printing strategy. It contains support structures for heat dissipation. A programmable furnace for additional heat treatment was installed nearby the printing unit. Furthermore, a dedicated software and milling machine was available for precision post-processing. Additive manufacturing is preceded by a digital model design. 3D printing is an additive manufacturing technology during which the metal-powder layers are added layer by layer, and the specimens are created with the structural fusion of these layers. The specimen model was designed in a 3D virtual environment and was followed by the printing process that lasted approximately four hours. After printing, specimens are removed from the machine and then separated from the building platform. The heat dissipating support material, which connects the specimens with the disc, is removed afterwards.

2.3. Heat treatment

Following the 3D printing procedure, specimens were subjected to heat treatment with parameters recommended by the manufacturer. **Figure 1.** shows the given heat treatment parameters obtained from the manufacturer. Heat-treating consists of three phases: heating, soaking, and cooling. The proper heat-treating technique is

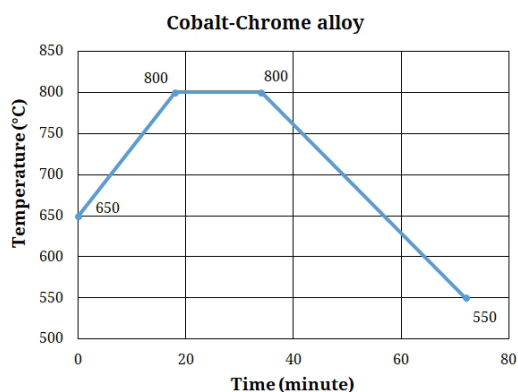


Figure 1. Heat-treating process provided by the manufacturer

chosen based on the size, geometry, material, and quality requirements of the given part. Hereby, the most important technological parameters can be defined, such as heat-treating temperature and cooling method.

3. Experiments

Using heat treatment parameters recommended by the manufacturer resulted in a brittle structure, which led to the fracture of some printed specimens. The heat-treating process parameters were changed after this. As a first approach, the heat treating temperature was changed. Numbers in **Table 2** label the following: number 1 indicates the heat treatment process provided by the manufacturer with a maximum temperature of 900°C. Numbers 2 and 4 represent heat-treating processes with a maximum temperature of 900°C. Numbers 3 and 5 mark 1050°C as the maximum temperature. At numbers 3 and 5, process times were changed. Here, all three phases of heat treatment were extended in time.

Changes were determined based on metallographic and experimental data.

Heat treatment marked with number 1 follows manufacturer's recommendations. Based on these experiments, number 4 shows the best solution so far, where fracture strain was increased the most. Thus, elastic modulus decreased, which meant the reduction of the brittleness of the whole structure. **Figure 2.** shows the process diagram for heat treatment labelled with number 4. Number 5 heat treatment had a temperature of 1050°C with a holding time of 118 minutes. No major differences were discovered, but surface oxidation occurred.

Hardness tests were then performed on the specimens. Rockwell hardness was measured in different points of the samples. **Table 3.** shows average hardness values characterizing the specimens.

Table 2. Mechanical properties obtained after testing

Number	Tensile strength (Mpa)	Fracture strain (%)	Elastic modulus (Mpa)
1	923	7.4	39 180
2	1041	7.2	47 362
3	1095	7.5	45 302
4	1003	16.06	33 804
5	1097	12.05	34 742

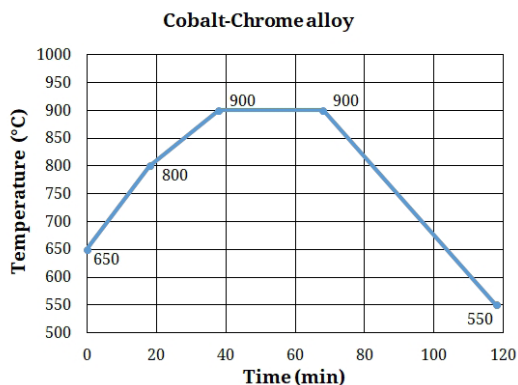


Figure 2. Heat treatment process

Table 3. Mechanical properties measured

Number	Hardness (HRC)
1	37.37
2	42.3
3	40.04
4	44.88
5	44.4

Table 3. shows the highest average hardness for the specimen marked with number 4. Hardness values measured on specimen number 4 also showed the lowest standard deviation. Other samples showed higher standard deviations during hardness tests. The next step of our research is influenced by the cause of these values.

4. Conclusion

Different heat treatment processes were presented in this study. Our goal was to obtain such mechanical properties for the additively manufactured cobalt-chromium alloy specimens that match dental requirements as precisely as possible. Elastic modulus, which provides information about the stiffness of the material, decreased. The study is going to be continued with the examination of different heat-treating processes. Partial results were achieved.

References

[1] Davis J. R.: *Nickel, cobalt and their alloys*. Materials. Park (OH), ASM International, 2000.

[2] Nasab M. B., Hassan M. R., Sahari B. B.: *Metallic biomaterials of knee and hip: a review*. Trends in Biomaterials and Artificial Organs, 24/2. (2010) 69–82.

<http://medind.nic.in/taa/t10/i2/taat10i2p69.pdf>

[3] Malayoglu U., Neville A.: *Mo and W, as alloying elements in Co-based alloy: their effects on erosion-corrosion resistance*. Wear, 259. (2005) 219–229.
<https://doi.org/10.1016/j.wear.2005.02.038>

[4] Monroy K., Delgadío J., Ciurana J.: *Study of the pore formation on CoCrMo alloys by selective laser melting manufacturing process*. Procedia Engineering, 63. (2013) 631–369.
<https://doi.org/10.1016/j.proeng.2013.08.227>

[5] Wataha J. C., Schmalz G.: *Dental alloys*. In: Biocompatibility of Dental Materials. (eds.: Schmalz G., Arenholt-Bindslev D.). Springer, Berlin, Heidelberg, 2009. 221–254.
https://doi.org/10.1007/978-3-540-77782-3_8

[6] Kalpana S. Katti: *Biomaterials in total joint replacement*. Colloid Surface B: Biointerfaces, 39/3. (2004) 133–142.
<https://doi.org/10.1016/j.colsurfb.2003.12.002>

[7] Hsu H. C., Lian S. S.: *Wear properties of Co-Cr-Mo-N plasma-melted surgical implant alloys*. Journal of Materials Processing Technology, 138. (2003) 231–235.
[https://doi.org/10.1016/S0924-0136\(03\)00077-3](https://doi.org/10.1016/S0924-0136(03)00077-3)

[8] Okazaki Y., Gotoh E.: *Comparison of metal release from various metallic biomaterials in vitro*. Biomaterials, 26/1. (2006) 11–21.
<https://doi.org/10.1016/j.biomaterials.2004.02.005>

[9] Lin H. Y., Bumgardner J. D.: *In vitro biocorrosion of Co-Cr-Mo implant alloy by macrophage cells*. Journal of Orthopaedic Research, 22/6. (2004) 1231–1236.
<https://doi.org/10.1016/j.orthres.2004.04.005>

[10] Hsu R. W-W., Yang C.-C., Huang C.-., Chenb Y.-S.: *Electrochemical corrosion studies on Cr-Co-Mo implant alloy in biological solutions*. Materials Chemistry and Physics, 93/2-3. (2005) 531–538.
<https://doi.org/10.1016/j.matchemphys.2005.04.007>

[11] Eggbeer D., Ribb R., Williams R.: *The computer-aided design and rapid prototyping fabrication of removable partial denture frameworks*. Proceedings of the Institution of Mechanical Engineers. Part H: Journal of Engineering in Medicine, 219/3. (2005) 195–202.
<https://doi.org/10.1243/095441105X9372>

[12] Dourandish M., Simchi A., Godlinski D.: *Rapid Manufacturing of Co-Cr-Mo Implants by Three-Dimensional Printing Process for Orthopedic Applications*. Iranian Journal of Pharmaceutical Sciences, 4/1 (2008) 31–36.
<https://pdfs.semanticscholar.org/9eef/39e-3f5ccb9b96171911b399044c201b66f12.pdf>

[13] Bertol L. S., Júnior W. K., da Silva F. P., Kopp C. A.: *Medical design: Direct metal laser sintering of Ti-6Al-4V*. Materials & Design, 31/8. (2010) 3983–3988.
<https://doi.org/10.1016/j.matdes.2010.02.050>

[14] Senthilkumaran K., Pandey P. M., Rao P. V. M.: *Influence of building strategies on the accuracy of*

parts in selective laser sintering. *Materials & Design*, 30/8. (2009) 2946–3294.

<https://doi.org/10.1016/j.matdes.2009.01.009>

- [15] Takaichi A., Nakamotoc T., Jokod N., Numorab N., Tsusumib Y., Migitab S. et al.: *Microstructures and mechanical properties of Co-29Cr-6Mo alloy fabricated by selective laser melting process for dental applications*. *Journal of the Mechanical Behavior of Biomedical Materials*, 21 (2013) 67–75.
<https://doi.org/10.1016/j.jmbbm.2013.01.021>

- [16] Nan X., Xian-Zhen X., Jie C., Bin W.: *Metal-ceramic bond strength of Co-Cr alloy, fabricated by selective laser melting*. *Journal of Dentistry*, 40/6. (2012) 453–457.

<https://doi.org/10.1016/j.jdent.2012.02.006>

- [17] Davis J. R. (Ed.): *Cobalt-Base Alloys*. In: *Handbook of Materials for Medical Devices*. ASM International, Ohio, 2003. 31–37.